


INL V	DRAWING RELEASE	KVG
0		

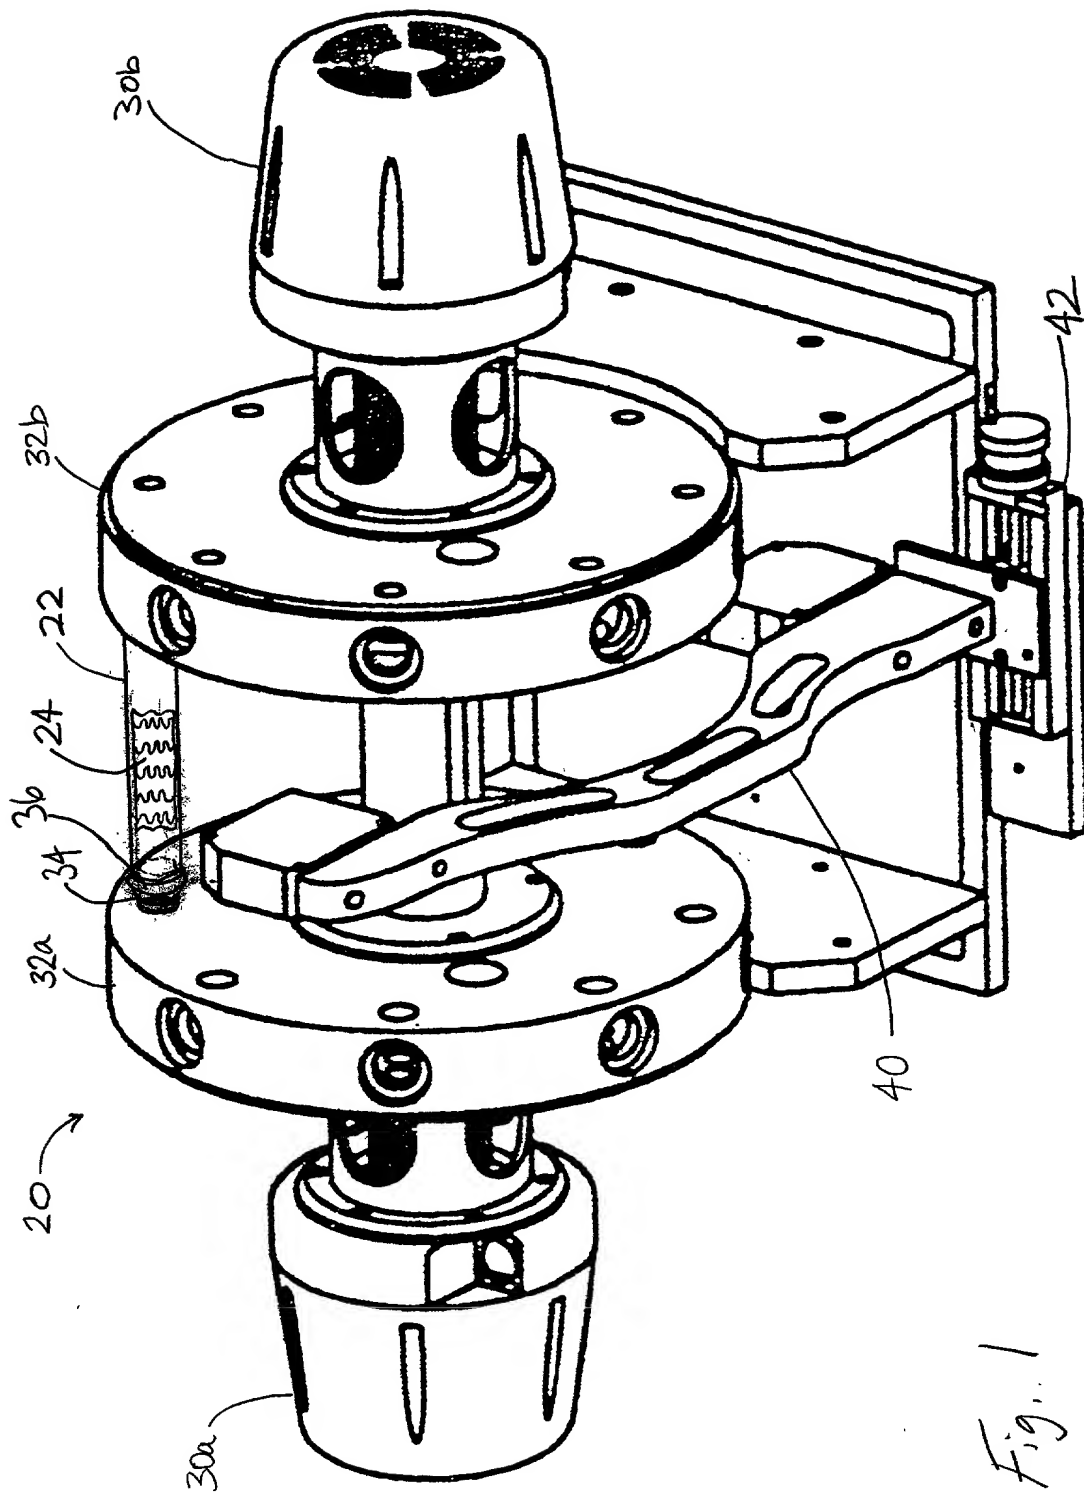

SCAIF 0 070

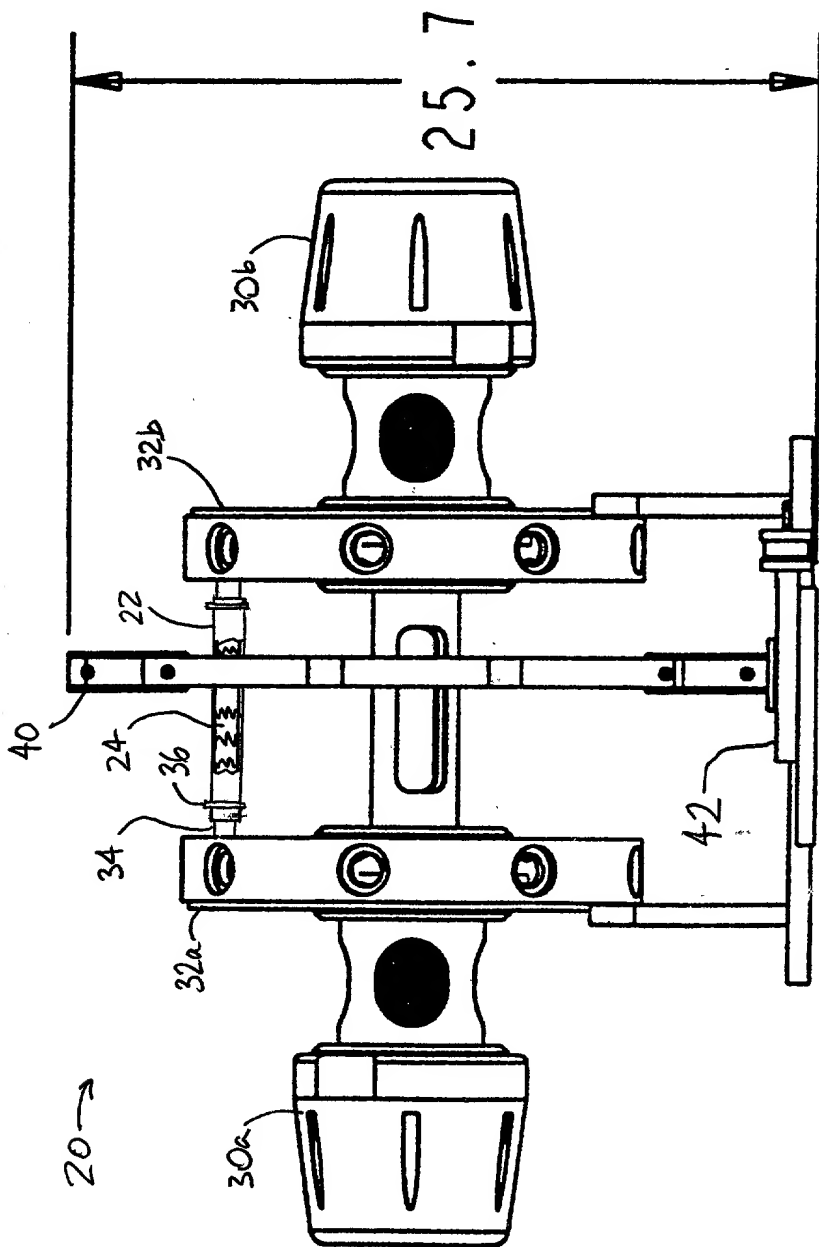
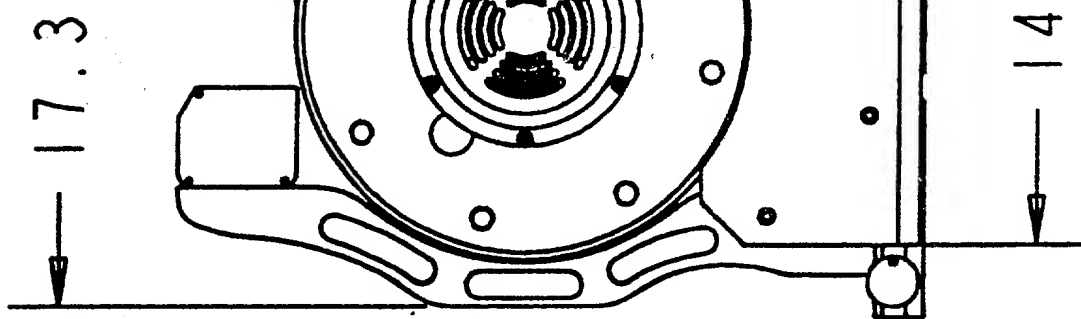



Fig. 2

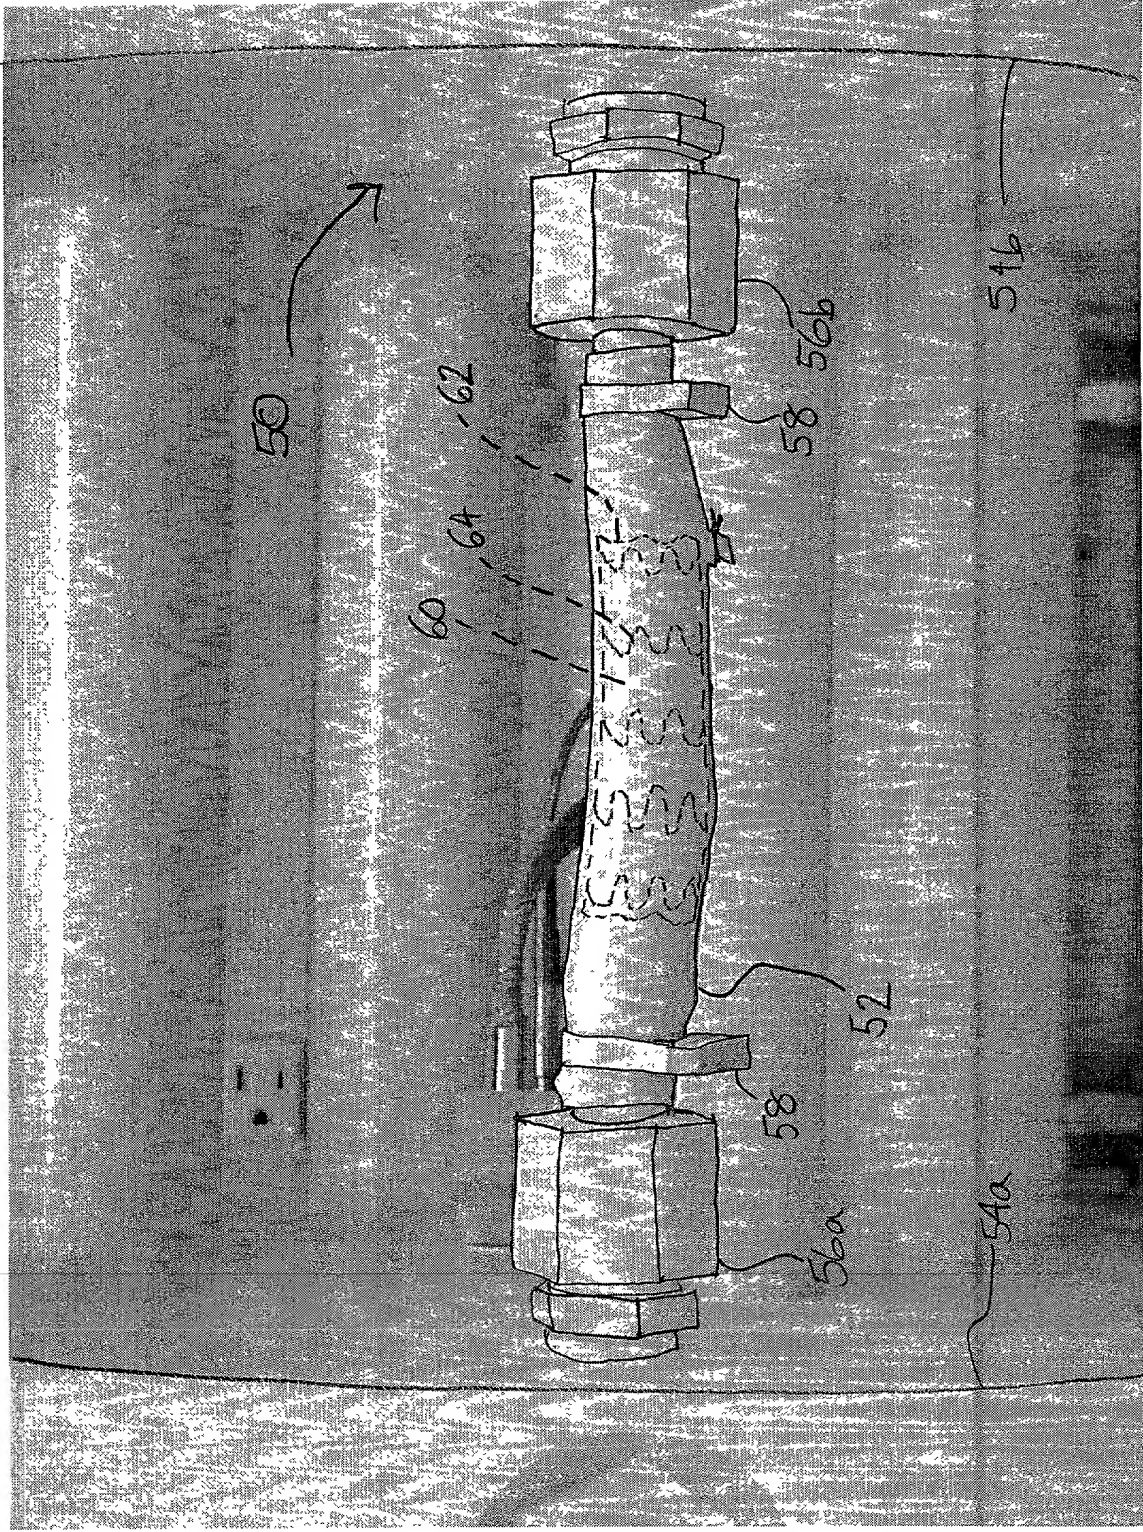


Fig. 3


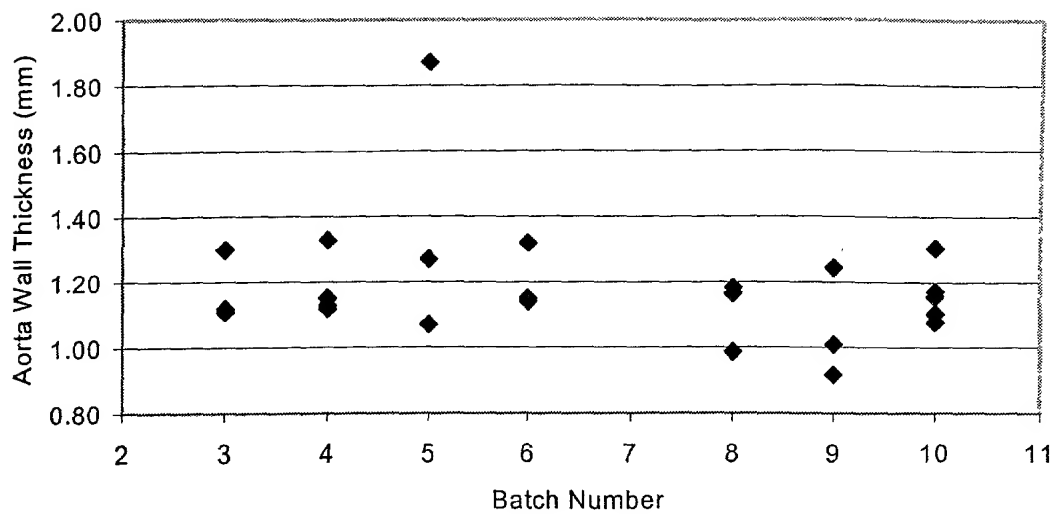


Fig. 4

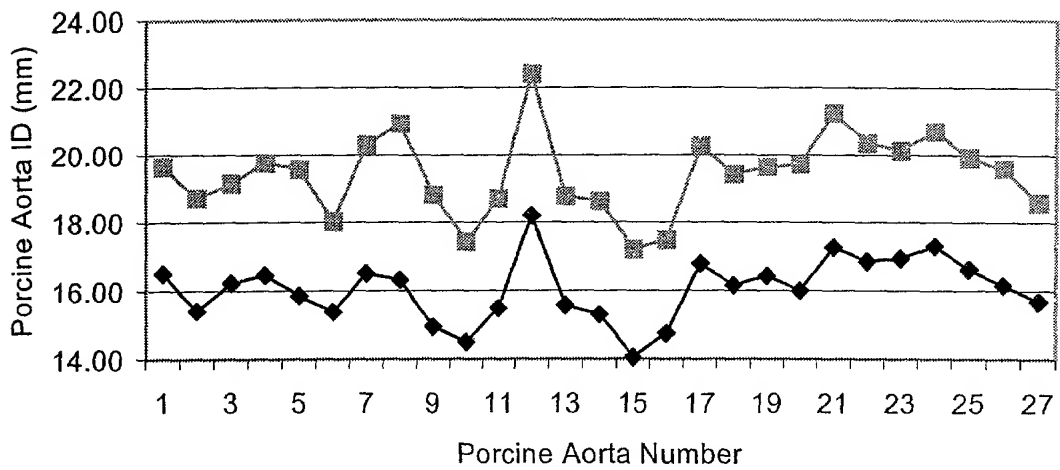

—◆— Aorta ID (mm) @ no external pressure —■— Aorta ID (mm) @ 100mmHg

Fig. 5

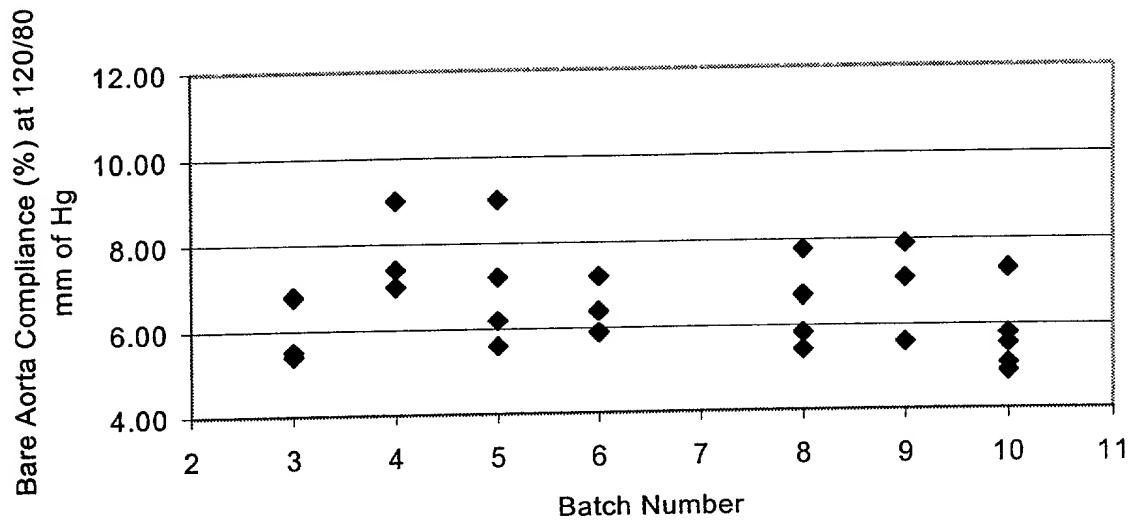


Fig. 6

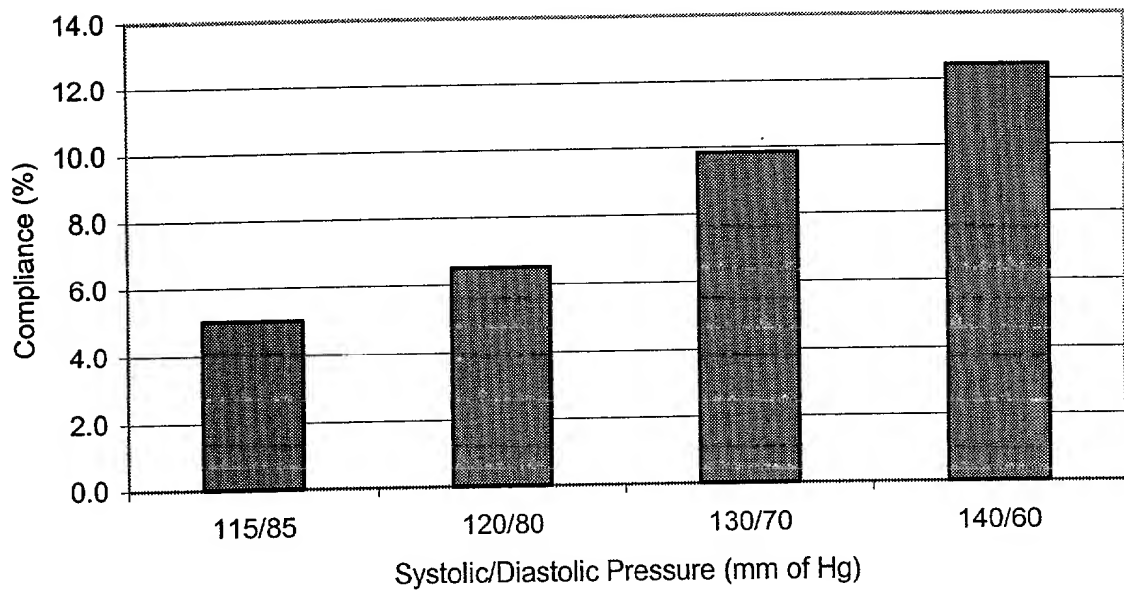


Fig. 7

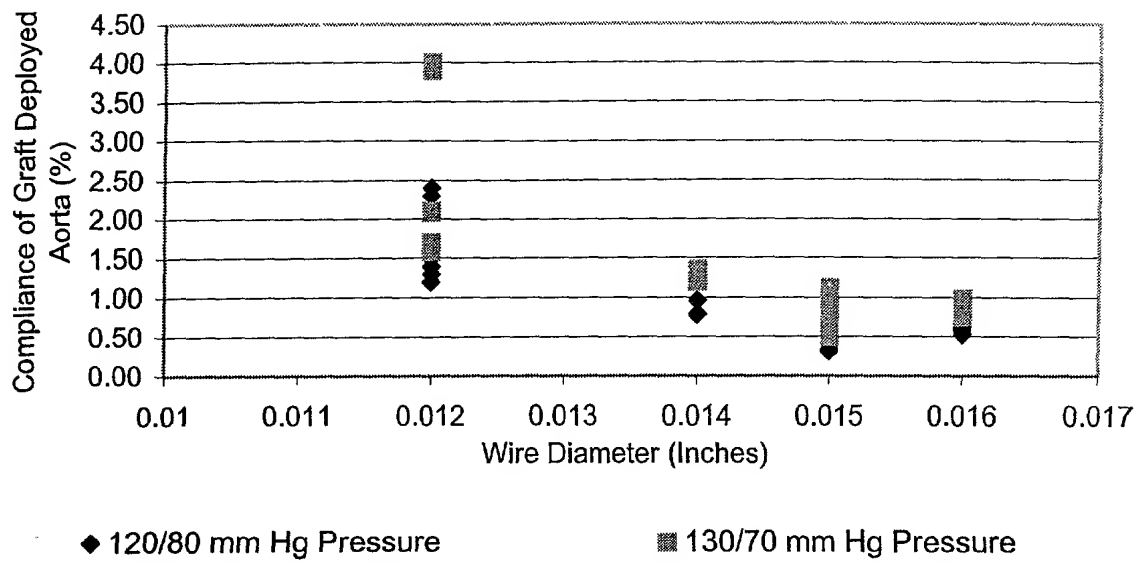


Fig. 8

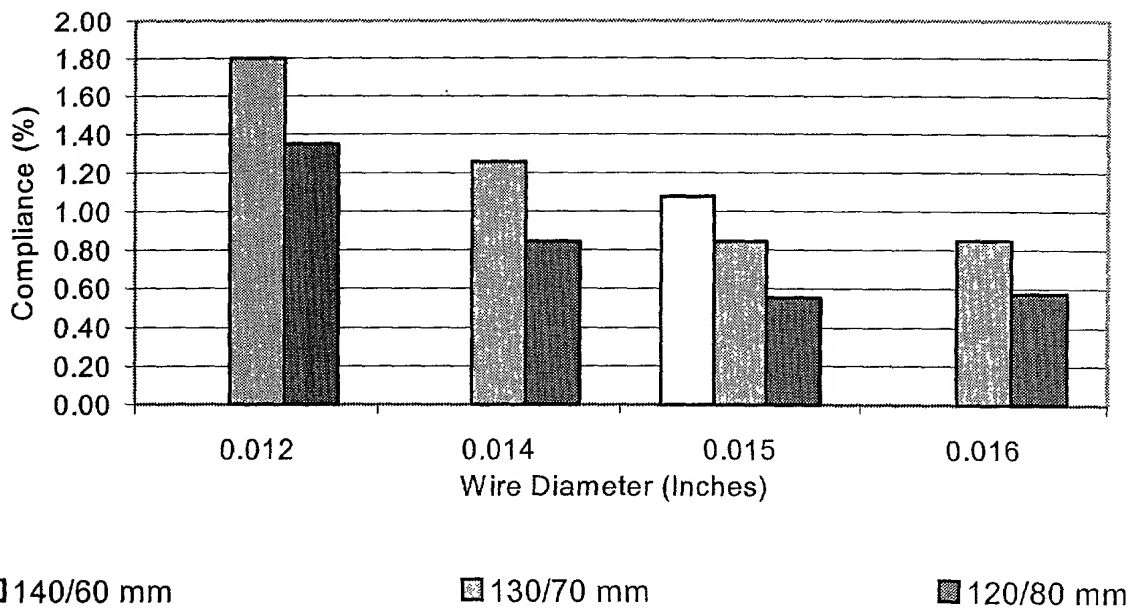


Fig. 9



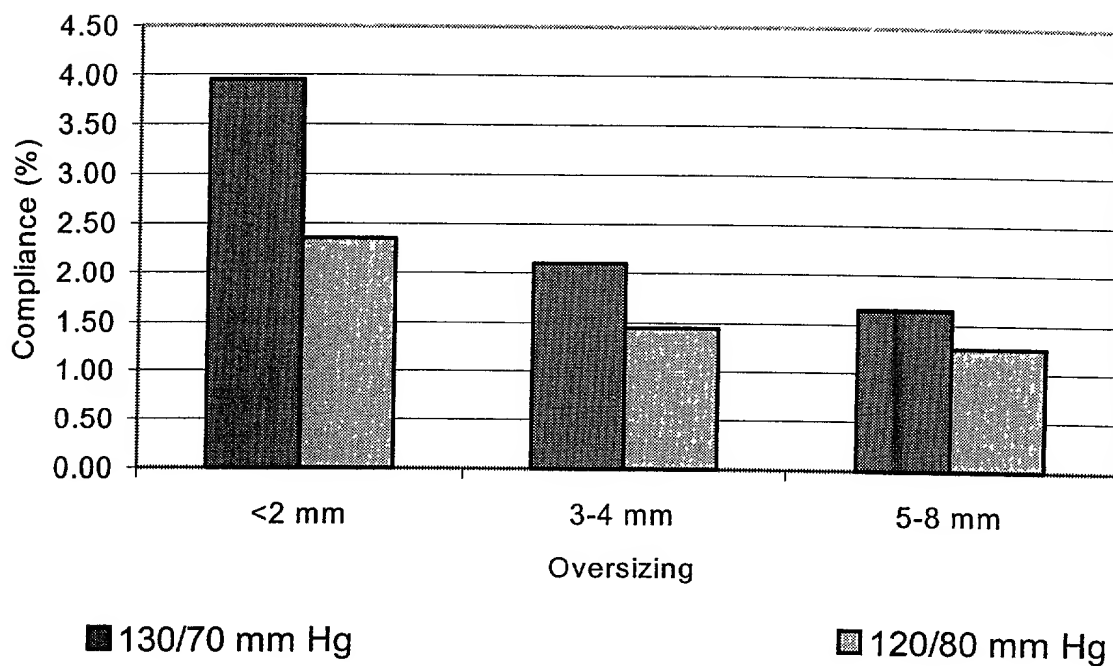


Fig. 10

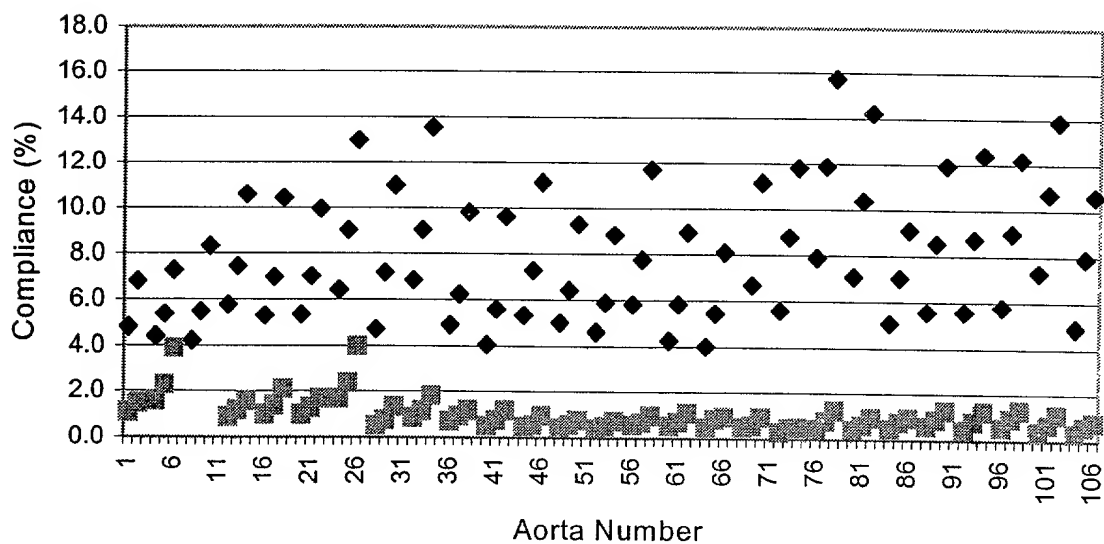

◆ Avg. Aorta Compliance without Graft (%) ■ Avg. Aorta Compliance with Graft Deploye

Fig. 11

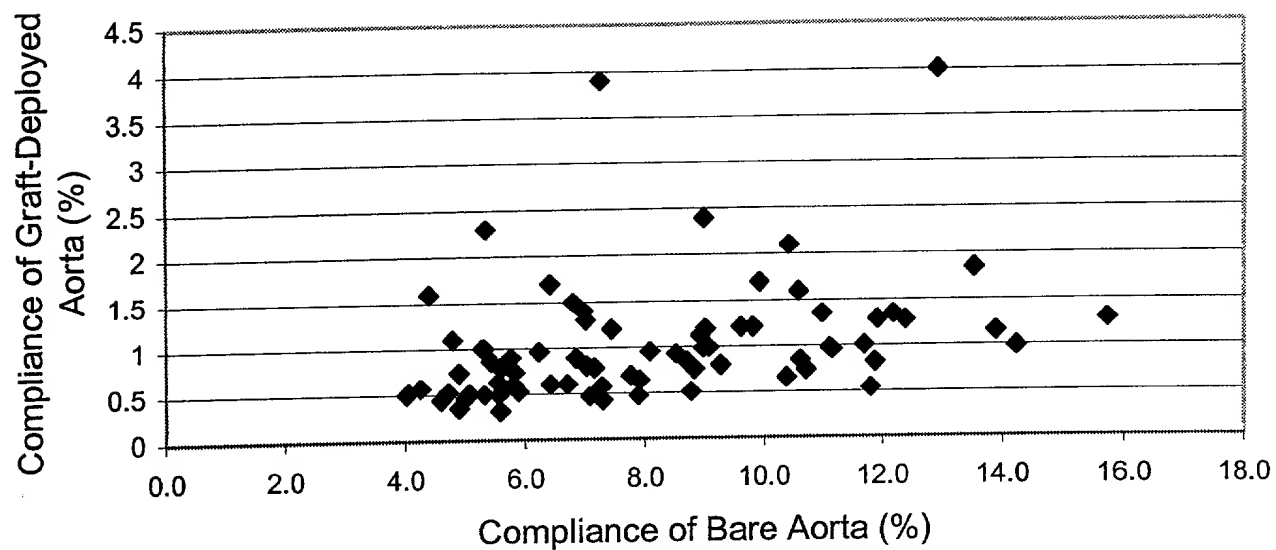

◆ 120/80 mmHg

Fig. 12